

HUMIDITY - TEMPERATURE - PRESSURE - WIND - PRECIPITATION - RADIATION



Instruction for Use

021410/08/04

Ultrasonic Anemometer

4.3804.00.540



ADOLF THIES GmbH & Co. KG

Hauptstraße 76
Box 3536 + 3541
Phone ++551 79001-0
www.thiesclima.com

37083 Göttingen Germany
37025 Göttingen
Fax ++551 79001-65
info@thiesclima.com

Contents

1	Models	3
2	Application	3
3	Mode of Operation	3
4	Measurement Principle	3
4.1	Wind speed and direction.....	3
4.2	Acoustic Virtual Temperature	4
5	Interface Description	5
5.1	Telegram forms	5
5.1.1	Telegram VD (STX)xx.x xxx*xx(CR)(ETX).....	5
5.1.2	Telegram VDT (STX)xx.x xxx xxx.x xx*xx(CR)(ETX)	6
5.1.3	Telegram V4DT (STX)xxx.x xxx xxx.x x xx*xx(CR)(ETX)	8
5.1.4	Telegram NMEA V 2.0 \$WIMWV,xxx.x,R,xxx.x,N,A*xx(CR)(LF).....	9
5.2	Definition of Checksum and Status byte	10
5.2.1	Forming of Checksum.....	10
5.2.2	Definition of Status byte.....	10
5.3	Telegram Output in Case of Error Events	11
6	Averaging Procedure	11
7	Standard Deviation	12
8	Bus – Ability, Synchronisation of the Measurement on the Query Telegram.....	12
8.1	Duplex - Mode	12
8.2	Synchronisation on Data Query	13
8.3	Averaging with Active Synchronisation	13
9	List of control commands	13
9.1	List of commands	14
9.2	Command Input.....	15
10	Recommendation Site Selection / Standard Installation.....	16
11	Installation	17
11.1	Mechanical Mounting	17
11.1.1	North Alignment.....	17
11.2	Electical Mounting	17
12	Maintenance	18
13	Calibration	18
14	Warranty	18
15	Technical Data.....	18
16	Dimension diagram.....	20
17	Accessories (Optional)	20

1 Models

Order no. with resp. model and factory setting see supplement sheet “Factory Setting”

2 Application

The **Ultrasonic Anemometer 2D** is designed to detect the horizontal components of wind speed and wind direction in two dimensions as well as the virtual temperature. Due to its very short measurement intervals, the instrument is ideal for the inertia-free measurement of gusts and peak values.

In certain weather situations the accuracy of the air temperature measurement (virtual-temperature) surpasses that one of the classic method where the temperature transmitter is used in a weather and thermal radiation shield.

The measured data are available as a data telegram via a serial interface.

The ultrasonic transducers as well as its carrying arms are automatically heated so that the measuring results, in case of critical ambient temperatures, are not affected by icing rain or snow.

3 Mode of Operation

The **Ultrasonic Anemometer 2D** consists of 4 ultrasonic transducers, in pairs of 2 which are opposite each other at a distance of 200 mm.

The two measurement paths thus formed are vertical to each other.

The transformers act both as acoustic transmitters and acoustic receivers.

The respective measurement paths and their measurement direction are selected via the electronic control. When a measurement starts, a sequence of 4 individual measurements in all 4 directions of the measurement paths is carried out at maximum possible speed.

The measurement directions (acoustic propagation directions) rotate clockwise, first from south to north, then from west to east, from north to south and finally from east to west.

The mean values are formed from the 4 individual measurements of the path directions and used for further calculations.

A measurement sequence takes approx. 10 m/sec at +20°C.

4 Measurement Principle

4.1 Wind speed and direction

The speed of propagation of the sound in calm air is superposed by the speed components of an air flow in wind direction.


A wind speed component in the direction of the propagation of the sound supports the speed of propagation, thus leading to an increase in the speed. A wind speed component opposite to the direction of propagation, on the contrary, leads to a reduction of the speed of propagation.

The speed of propagation resulting from the superposition leads to different propagation times of the sound at different wind velocities and directions over a fixed measurement path.

As the speed of sound is very dependent on the air temperature, the propagation time of the sound is measured on both of the measurement paths in both directions. In this way, the influence of the temperature-dependent speed of sound on the measurement result can be eliminated.

By combining the two measuring paths which are at right angles to each other, one obtains the measurement results of the sum and the angle of the wind speed vector in the form of rectangular components.

After the rectangular speed components have been measured, they are then transformed by the μ -processor of the anemometer into polar co-ordinates and output as sum and angle of wind speed.

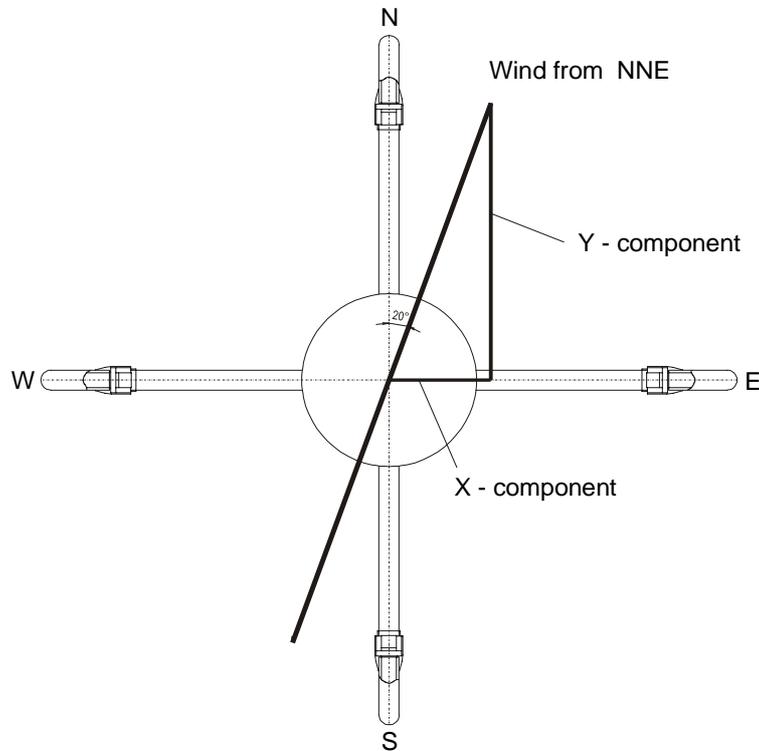

4.2 Acoustic Virtual Temperature

As previously mentioned, the speed of the propagation of sound is shows a radix dependency on the absolute air temperature, but is rather independent of air pressure, and only slightly dependent of humidity. Thus these physical properties of gases can be used to measure air temperature at constant and known chemical composition.

It is a measurement of gas temperature which is made without thermal coupling to a solid state sensor.

The advantages of this measured variable is, on the one hand, its inertia free reaction to the actual gas temperature, and, on the other hand, the avoidance of measurement errors such as those which occur when a solid state temperature sensor is heated up by radiation.

Due to the low dependency of the speed of propagation of the sound on the air humidity, the "Virtual Temperature" refers to dry air (0% humidity) under the same pressure conditions as that one actually measured.

The deviation of the measured "acoustic-virtual temperature", compared with the real air temperature, is linear-dependent from the absolute humidity content of the air.

The part of water vapour in the air increases proportionally the sonic speed, as H₂O-molecules have approx. only half of the mass of the remaining air-molecules (O₂ and N₂).

The rise of the sonic speed leads to an apparent (virtual) rising of the measured temperature in

humid air compared with dry air of the same temperature.

The deviation of the measured virtual temperature in humid air, compared with real air temperature, can be corrected according to the following correlation, when the value of absolute humidity is given:

$$T_r = T_v - 0,135 \text{ K} * \text{m}^3 / \text{g} * a$$

and T_r represents the real air temperature, T_v the measured acoustic-virtual temperature and a the absolute humidity in grams H_2O per m^3 of air.

5 Interface Description

5.1 Telegram forms

5.1.1 Telegram VD (STX)xx.x xxx*xx(CR)(ETX)

Z. Nr.	Function
1	STX (HEX 02)
2	10^1 Wind speed
3	10^0 Wind speed
4	“.” Decimal point
5	10^{-1} Wind speed
6	space (HEX 20)
7	10^2 Wind direction
8	10^1 Wind direction
9	10^0 Wind direction
10	* (HEX 2A) Check sum identifier
11	High Byte check sum in HEX
12	Low Byte check sum in HEX
13	CR (HEX 0D) Carriage return
14	ETX (HEX 03)

5.1.2 Telegram VDT

(STX)xx.x xxx xxx.x xx*xx(CR)(ETX)

Z. Nr.	Function
1	STX (HEX 02)
2	10 ¹ Wind speed
3	10 ⁰ Wind speed
4	“.” (HEX 2E) Decimal point
5	10 ⁻¹ Wind speed
6	Space (HEX 20)
7	10 ² Wind direction
8	10 ¹ Wind direction
9	10 ⁰ Wind direction
10	Space (HEX 20)
11	+ or - sign
12	10 ¹ Temperature
13	10 ⁰ Temperature
14	“.” (HEX 2E) Decimal point
15	10 ⁻¹ Temperature
16	Space (HEX 20)
17	High Byte status byte
18	Low Byte status byte
19	* (HEX 2A) Check sum identifier
20	High Byte Check sum in HEX
21	Low Byte Check sum in HEX
22	CR (HEX 0D) Carriage return
23	ETX (HEX 03)

5.1.2.1 Telegram VDT (STX)xx.x xxx xxx.x xx*xx xx.x xxx(CR)(ETX)

When using the standard deviation the VDT-telegram is extended by the standard deviations of wind speed and wind direction.

Z. Nr.	Function
1	STX (HEX 02)
2	10 ¹ Wind speed
3	10 ⁰ Wind speed
4	. (HEX 2E) Decimal point
5	10 ⁻¹ Wind speed
6	Space (HEX 20)
7	10 ² Wind direction
8	10 ¹ Wind direction
9	10 ⁰ Wind direction
10	Space (HEX 20)
11	+ or - sign
12	10 ¹ Temperature
13	10 ⁰ Temperature
14	. (HEX 2E) Decimal point
15	10 ⁻¹ Temperature
16	Space (HEX 20)
17	10 ¹ Wind speed (Standard deviation)
18	10 ⁰ Wind speed (Standard deviation)
19	. (HEX 2E) Decimal point
20	10 ⁻¹ Wind speed (Standard deviation)
21	Space (HEX 20)
22	10 ² Wind direction (Standard deviation)
23	10 ¹ Wind direction (Standard deviation)
24	10 ⁰ Wind direction (Standard deviation)
25	Space (HEX 20)
26	High Byte statusbyte
27	Low Byte statusbyte
28	* (HEX 2A) Check sum identifier
29	High Byte Check sum in HEX
30	Low Byte Check sum in HEX
31	CR (HEX 0D) Carriage Return
32	ETX (HEX 03)

5.1.3 Telegram V4DT

(STX)xxx.x xxx xxx.x x xx*xx(CR)(ETX)

Z. Nr.	FunCtion
1	STX (HEX 02)
2	10 ² Wind speed
3	10 ¹ Wind speed
4	10 ⁰ Wind speed
5	. (HEX 2E) Decimal point
6	10 ⁻¹ Wind speed
7	Spare (HEX 20)
8	10 ² Wind direction
9	10 ¹ Wind direction
10	10 ⁰ Wind direction
11	Space (HEX 20)
12	+ or - Sign
13	10 ¹ Temperature
14	10 ⁰ Temperature
15	. (HEX 2E) Decimal point
16	10 ⁻¹ Temperature
17	Space (HEX 20)
18	K, N, M, S = km/h, Knots, m/s, mph
19	Space (HEX 20)
20	High Byte Status byte
21	Low Byte Status byte
22	* (HEX 2A) Check sum identifier
23	High Byte Check sum in HEX
24	Low Byte Check sum in HEX
25	CR (HEX 0D) Carriage return
26	ETX (HEX 03)

5.1.4 Telegram NMEA V 2.0

\$WIMWV,xxx.x,R,xxx.x,N,A*xx(CR)(LF)

Z. Nr.	Function
1	\$ (HEX 24) Dollar
2	W (HEX 57)
3	I (HEX 49)
4	M (HEX 4D)
5	W (HEX 57)
6	V (HEX 56)
7	, (HEX 2C) Comma
8	10 ² Wind direction
9	10 ¹ Wind direction
10	10 ⁰ Wind direction
11	. (HEX 2E) decimal point
12	10 ⁻¹ Wind direction
13	, (HEX 2C) Comma
14	R (HEX 52)
15	, (HEX 2C) Comma
16	10 ² Wind speed
17	10 ¹ Wind speed
18	10 ⁰ Wind speed
19	. (HEX 2E) Decimal point
20	10 ⁻¹ Wind speed
21	, (HEX 2C) Comma
22	K, N, M, S = km/h, Knots, m/s, mph
23	, (HEX 2C) Comma
24	A, V A = valid, V = non valid
25	* (HEX 2A) Check sum identifier
26	High Byte Check sum in HEX
27	Low Byte Check sum in HEX
28	CR (HEX 0D) Carriage Return
29	LF (HEX 0A) Line Feed

5.3 Telegram Output in Case of Error Events

In the following cases the digital telegram outputs „F“ as measurement value figure instead of numbers:

- If the measurement acquisition is constantly disturbed for more than 10 seconds in spite of multiple measurements
- If the deviation of the virtual temperature between both measurement paths is > 8 K.

6 Averaging Procedure

The Ultrasonic 2D forms the gliding mean value through a FIFO-memory the capacity of which comprises up to 600 values.

In the free running measurement mode the measurement data rate is exactly 10 Hz or 100msec, and forms, at the same time, the updating rate for the averaging memory (FIFO-memory).

If averaging is requested the measured data are recorded in the FIFO-memory stated above, the capacity of which is built-up depending on the selected averaging period.

If the averaging period is, for example, 10 seconds, 100 memory cells are used, and in case of an averaging period of 1 minute 600 cells.

From a selected averaging period > 1 minute up the data flow will be pre-averaged; because the memory capacity of 600 values cannot be exceeded.

The Ultrasonic 2 D combines two different and useful procedures of mean value forming:

- The forming of vectorial mean values
- The forming of scalar mean values

These different procedures can be selected for the averaging of both the wind speed and wind direction, depending on the application.

The procedure of forming the vectorial mean value takes the wind direction into account when averaging the wind speed and vice versa.

Thus, the averaged dimensions of wind speed and wind direction are valued each one with the other.

This procedure of forming the mean value is well suited, for example, for measurements and analysis of pollutant-propagation.

The procedure of forming the scalar mean value averages both dimensions of wind speed and wind direction independently from each other.

These averaging procedures lead to results comparable with mechanical wind speed- and wind direction transmitters.

The scalar averaging procedure is suited, for example, for location-analysis for wind power plants, where only the dimension of the wind vector – important for power generation – is interesting but not its direction.

The vectorial and scalar procedure can be used independently with wind speed and wind direction within an output telegram.

For this, you have to select one of the four possible combinations through the command **AM (Average Method)**.

Command for selecting the averaging procedure:

AM00000 (Average Method) vectorial averaging of speed and direction

AM00001 scalar averaging of speed and direction

AM00002 scalar averaging of speed and vectorial averaging of direction

AM00003 vectorial averaging of speed and scalar averaging of direction

7 Standard Deviation

Starting with the firmware version V 1.8 the ULTRASONIC is capable to calculate the standard deviation. The standard deviation for wind speed and wind direction is determined at an averaging period of > 1 sec. The calculation is carried out in accordance with the following formula:

$$Y = \sqrt{\frac{1}{n} \sum_{i=0}^{i<n} (\bar{M} - Xi)^2} \quad \text{mit} \quad \bar{M} = \frac{1}{n} \sum_{i=0}^{i<n} Xi$$

The standard deviation is activated through the command "DE00001". It is important that the ULTRASONIC reduces the measuring interval to 50 hz when calculating the standard deviation. This is necessary for the instrument to finish the calculations of the standard deviations between two measuring cycles. The calculation of the standard deviation is activated when the selected averaging period is > 1sec.

8 Bus – Ability, Synchronisation of the Measurement on the Query Telegram

8.1 Duplex - Mode

The Ultrasonic supports absolutely any operation at an RS485/RS422 data bus in co-operation with further instruments (bus operation).

Supported are both semi-duplex bus-topologies and full duplex bus-systems.

In the semi- and full duplex operation the line drivers of the Ultrasonic are active only for the time of data transmission.

The remaining time the line drivers are off-line ("three-state-mode").

The direct connection to a PC with RS232 interface makes an interface-converter RS 485 / RS 232 necessary, e.g. our accessories order-no. 9.1702.20.000

Command for Selecting the duplex-mode (DM for duplex mode):

DM00000 for semi-duplex (2-wire operation)

DM00001 for full duplex (4-wire operation) (state of delivery).

In case of bus operation a spontaneous output of the Ultrasonic is suppressed – the instruments respond only on request of the bus master.

When semi-duplex operation is set, a spontaneous telegram output is not selectable.

In case the spontaneous telegram output has been selected erroneously this could lead to a blocking of the receivers at slow baud rates.

8.2 Synchronisation on Data Query

Certain application make it necessary to interrogate cyclically a collective of instruments within a short time (e.g. 5 instruments within 100 ms).

There might be the following problem: the Ultrasonic can be contacted during a measurement by the asynchronous query and is then not ready for transmission.

In order to guarantee an immediate instrument response without delay, the possibility of temporal measurement synchronisation on the query is used.

Command for activating the ability for measurement-synchronisation on the query:

MT00001 (Measurement Trigger) Synchronisation Ability on.

MT00000 Synchronisation Ability off.

In case the instrument receives, with active synchronisation, a telegram inquiry through the command TR0000x, and further inquiry follow with intervals of less than 2,5 seconds, the instrument runs synchronously to the inquiries and responds with smallest possible delay. If there are no queries for more than 2,5 seconds, the instrument leaves the synchronous mode and changes into a spontaneous measurement value acquisition.

This return to the spontaneous mode of measurement guarantees that all control functions derived from the measurement data (e.g. switch-on heating etc.) will be able to operate also in case of a failure of query telegram.

As soon as a new query occurs in the spontaneous mode the instrument synchronises immediately on the query telegram.

8.3 Averaging with Active Synchronisation

In case the measurement values should be averaged please take care that – with active synchronisation – the exact, internal time basis of 100 ms for forming the measurement values is not used. In this case, the time is determined by the query-repetition-rate.

It is advisable to switch-off the synchronisation ability if it is not absolutely necessary.

9 List of control commands

The Anemometer 2D can be controlled via its serial data interface using the commands in the following list.

Any standard terminal program such as “procomm“ , “telix“ or a *Windows* terminal program (e.g. “Hyper Terminal”) can be used.

All adjustments are stored in a E²ROM so that the adjusted parameters cannot get lost after switching off or failure of power supply.

9.1 List of commands

Command	Function	Remark
<ID> AM 00000	Vectorial averaging	Vectorial averaging of wind speed and direction
<ID> AM 00001	Scalar averaging	Scalar averaging of wind speed and direction
<ID> AM 00002	Scalar / vectorial averaging	Scalar averaging of speed / vectorial averaging of direction
<ID> AM 00003	Vectorial / Scalar averaging	Vectorial averaging of speed / scalar averaging of direction
<ID> AV 00000	Instantaneous value	Output of the instantaneous values
<ID> AV 00001	Mean value over 1 second	Output of the gliding mean value over 1 second
<ID> AV 00002	Mean value over 10 seconds	Output of the gliding mean value over 10 seconds
<ID> AV 00003	Mean value over 1 minute	Output of the gliding mean value over 1 minute
<ID> AV 00004	Mean value over 2 minutes	Output of the gliding mean value over 2 minutes
<ID> AV 00005	Mean value over 10 minutes	Output of the gliding mean value over 10 minutes
<ID> BR 00002	1200 Baud N 8 1	Data rate 1200 Baud, 8 Data bits, No Parity, 1 Stop bit
<ID> BR 00010	1200 Baud E 7 1	Data rate 1200 Baud, 7 Data bits, Parity Equal, 1 Stop bit
<ID> BR 00003	2400 Baud N 8 1	Data rate 2400 Baud, 8 Data bits, No Parity, 1 Stop bit
<ID> BR 00011	2400 Baud E 7 1	Data rate 2400 Baud, 7 Data bits, Parity Equal, 1 Stop bit
<ID> BR 00004	4800 Baud N 8 1	Data rate 4800 Baud, 8 Data bits, No Parity, 1 Stop bit
<ID> BR 00012	4800 Baud E 7 1	Data rate 4800 Baud, 7 Data bits, Parity Equal, 1 Stop bit
<ID> BR 00005	9600 Baud N 8 1	Data rate 9600 Baud, 8 Data bits, No Parity, 1 Stop bit
<ID> BR 00013	9600 Baud E 7 1	Data rate 9600 Baud, 7 Data bits, Parity Equal, 1 Stop bit
<ID> BR 00006	19200 Baud N 8 1	Data rate 19200 Baud, 8 Data bits, No Parity, 1 Stop bit
<ID> BR 00014	19200 Baud E 7 1	Data rate 19200 Baud, 7 Data bits, Parity Equal, 1 Stop bit
<ID> DE 00000	Standard deviation of	De-activate calculation of the standard deviation
<ID> DE 00001	Standard deviation on	Activate calculation of the standard deviation
<ID> DM 00000	Duplex mode half duplex (HD)	Half duplex, 2-wire operation
<ID> DM 00001	Duplex mode full duplex (FD)	Full duplex, 4-wire operation
<ID> DV	Firmwareversion	Release of firmware version
<ID> ES 00000	Sign-echo switched off	Echo operation of transmitted characters switched off
<ID> ES 00001	Sign-echo switched on	Echo operation of transmitted characters switched on
<ID> KY 00000	Key, no access	Software-key, access to EEPROM closed
<ID> KY 00001	Key, open access	Software- key, access to EEPROM open
<ID> MT 00000	Measurement trigger off	No synchronization of measurement onto request poss.
<ID> MT 00001	Measurement trigger on	Synchronization of measurement onto request possible

<ID> NC 00xxx	North correction in 1°	Input of north correction, value range 00000 up to 00360
<ID> OR 00xxx	Output rate online (spontaneous)	Output rate xxx times 100ms, value range 00001 up to 00255
<ID> OS 00000	Wind speed in m/s	Scale of Wind speed in meter per second
<ID> OS 00001	Wind speed in Km/h	Scaling of Wind speed in kilo meter per hour
<ID> OS 00002	Wind speed in mph	Scaling of Wind speed in miles per hour
<ID> OS 00003	Wind speed in Knots	Scaling of Wind speed in knots (nautically)
<ID> TR 00001	Telegram VD on request	single output of the telegram form, see 6.1.1
<ID> TR 00002	Telegram VDT on request	single output of the telegram form, see 6.1.2
<ID> TR 00003	Telegram V4DT on request	single output of the telegram form, see 6.1.3
<ID> TT 00000	No telegram output	
<ID> TT 00001	Telegram VD spontaneous	Online output of telegram form, see 6.1.1
<ID> TT 00002	Telegram VDT spontaneous	Online output of telegram form, see 6.1.2
<ID> TT 00003	Telegram V4DT spontaneous	Online output of telegram form, to 6.1.3
<ID> TT 00004	Telegram NMEA V 2.0	Online output of telegram form, to 6.1.4

Remark:

■ *Due to the compatibility the telegrams VD and VDT supply the wind speed in 3 digits form.
In order to avoid that the measuring range is exceeded the telegrams deliver the wind speed exclusively in the unit of m/s (meters per second)!*

9.2 Command Input

Please find your ID (identifier-number) in the works certificate included in the delivery.

For the input of commands and parameters please open first the access to the EEPROM by entering the command (ID) KY00001.

After all inputs have been made the access to the EEPROM should be locked again through the command (ID) KY00000 in order to avoid unauthorised changes of the system parameters.

The command is input by entering the instrument identification number (ID) followed by two letters which specify the actual command followed by a 5-digit code number respective value.

The characters are entered **without a space** and are **activated with Return**.

Entering the command without the 5-digit code number is interpreted as a query of the command status and leads to the output of the current command status.

Correcting the command word during input when an error has occurred is **not allowed** and the command will not be accepted.

All letters must be **capitalised**, otherwise they will not be accepted.

11 Installation

11.1 Mechanical Mounting

The wind transmitter must be mounted to a pipe piece of R 1 ½" (Ø 48.3 mm) which is 50 mm long. The internal diameter of the pipe must be at least 30 mm as the wind transmitter is connected electrically from below with a cable. Solder a flexible control line LiYCY with the corresponding number of cores to the enclosed plug. After the wind transmitter has been connected, set it onto the pipe piece respectively the mast piece. The branch of the red marked sonic transducer must be aligned to North. To do this, take a bearing via the ultrasonic transducer of the North/South path onto an object to the North, for example a building or a special geographic feature. Use the four screws with hexagonal recessed holes (SW 4 mm) to attach the instrument to the shaft.

Note:

When using a lightning rod please take care that it is mounted always in an angle of 45° to the measuring distance, as otherwise there might be deviations of measuring value.

11.1.1 North Alignment

For the alignment of the anemometer the **branch of the red marked sonic transducer must indicate to North**. For this, you select an obvious point in a northerly or southerly direction in the surroundings with the aid of a compass; then turn the mast or the anemometer into this direction until both arms opposite are situated in a straight line.

It is also possible that oneself stands in a northerly or southerly direction with respective distance, and a partner turns the anemometer or mast by command until both sensor arms are situated in a straight line. In this case, it is advisable to use a pair of field glasses.

11.2 Electrical Mounting

Wire colour	Function	Remark
brown	TX+ (Y)	serial interface
yellow	RX+	serial interface
green	RX-	serial interface
white	TX- (Z)	serial interface
black 1	Power electronics 12-24V AC/DC	
black 2	Power electronics 12-24V AC/DC	
black 3	Power heater / electronics 24V AC/DC	
black 4	Power heater / electronics 24V AC/DC	

12 Maintenance

As the instrument has no moving parts i.e. operates without wear or tear, only minimal maintenance is required. As the sensor surface is permanently washed up by the falling rain it is only occasionally necessary to clean the surface with non-aggressive cleansing agent and soft cloth. These cleansing activities can be carried out – as far as necessary – on occasion of the routine checks.

13 Calibration

The ultrasonic anemometer does not contain any adjustable components such as electrical or mechanical trimming elements. All of the components and materials are invariant in time. Thus, regular calibration because of ageing is not required. Only a mechanical deformation of the transformer arms and the resulting changes in the length of the measurement paths lead to errors in the measured values.

The virtual temperature can be used to check the length of the measurement path. A change in the measurement path length of 0.17% and consequently a measurement error of 0.17% of the wind speed corresponds to a 1 K deviation of the virtual temperature at 20 °C, thus at 6 K deviation, the measurement error of wind speed is approx. 1%.

If the distance of measuring path of the anemometer is de-aligned please contact the producer for a re-calibration of the instrument.

14 Warranty


Damages resulting from improper handling or caused by external influences, e.g. lightning, are excluded from the warranty. The warranty expires if the instrument has been opened.

15 Technical Data

Wind Speed	Meas. range	0...65 m/s
	Accuracy	± 0.1 m/s , at the range 0 ... 5 m/s resp. ± 2 % rms from meas. value , at > 5 m/s
	Resolution	0.1 m/s
Wind Direction	Meas. range	0...360°
	Accuracy	$\pm 1.0^\circ$
	Resolution	1°
Virtual Temperature	Meas. range	- 40 + 70 °C
	Accuracy	± 0.5 K
	Resolution	0.1 K

Data output	digital	Interface	RS 485
		Baud rate	1200, 2400, 4800, 9600, 19200 selectable
		Output	Instantaneous values of speed, direction and Virtual -temperature. Gliding mean values 1sec.; 10sec.; 1min.; 2min.; 10min.
		Output rate	1 per 100 m/sec up to 1 per 25.5 sec, selectable
		Status identification	Heater status, Path disturbance, temperature deviation path to path > 8 Kelvin
General		Internal meas. rate	400 measurements per second, at 25 °C
		Temp. range	- 40 ... + 70 °C
		Supply voltage	electronics, 12 ... 24 V AC/DC ± 10%, max. 3 VA
			heater , 24 V AC/DC ± 10%, max. 70 VA
		Protection	IP 66
		Icing	acc. to THIES STD 012001
		Corrosion	No corrosion after 3 month of salt fog and condensation
		EMV	EN 55022 5/95 class B; EN50082-2 2/96
		Model	Stainless 1.4571 steel for housing and sensor arms
		Mounting	to a mast tube 1 ½ ", for ex. DIN 2441
		Type of connection	8 pole cable 211858, 2.2 m long
		Weight	approx. 2.5 kg

16 Dimension diagram

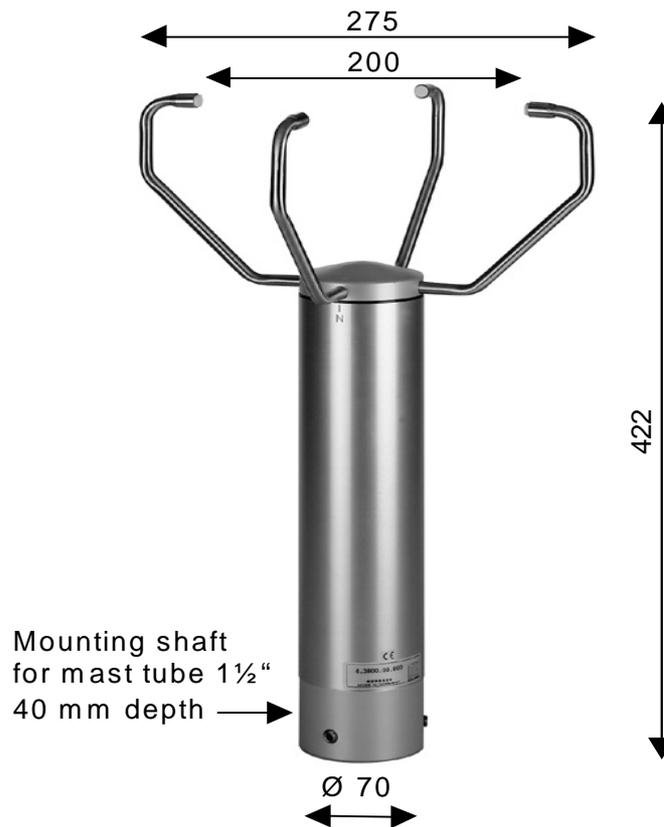

17 Accessories (Optional)

PC Software Meteo-Online	9.1700.98.000	For visualization of data on PC screen
Power Supply Unit	9.3388.00.000	For the power supply of the Ultrasonic
RS 232 / RS 422 converter	9.1702.20.000	For signal conversion of RS 422 in RS 232
Lightning Rod	4.3100.99.150	For lightning protection

Attention:

■ **A return of the instruments must be effected in the original packing as otherwise the guarantee expires in case of mechanical damages e.g. by deformation of the transducer arms.**



ADOLF THIES GmbH & Co. KG

Hauptstraße 76 37083 Göttingen Germany
 P.O. Box 3536 + 3541 37025 Göttingen
 Phone ++551 79001-0 Fax ++551 79001-65
 www.thiesclima.com info@thiesclima.com



- Alterations reserved -